

SURESTEP[®]

FOLEY CATHETER SYSTEM

Following the directions is as easy as A, B, C.


A) Always clean the patient



B) Be sure to use aseptic technique



C) Care and maintenance

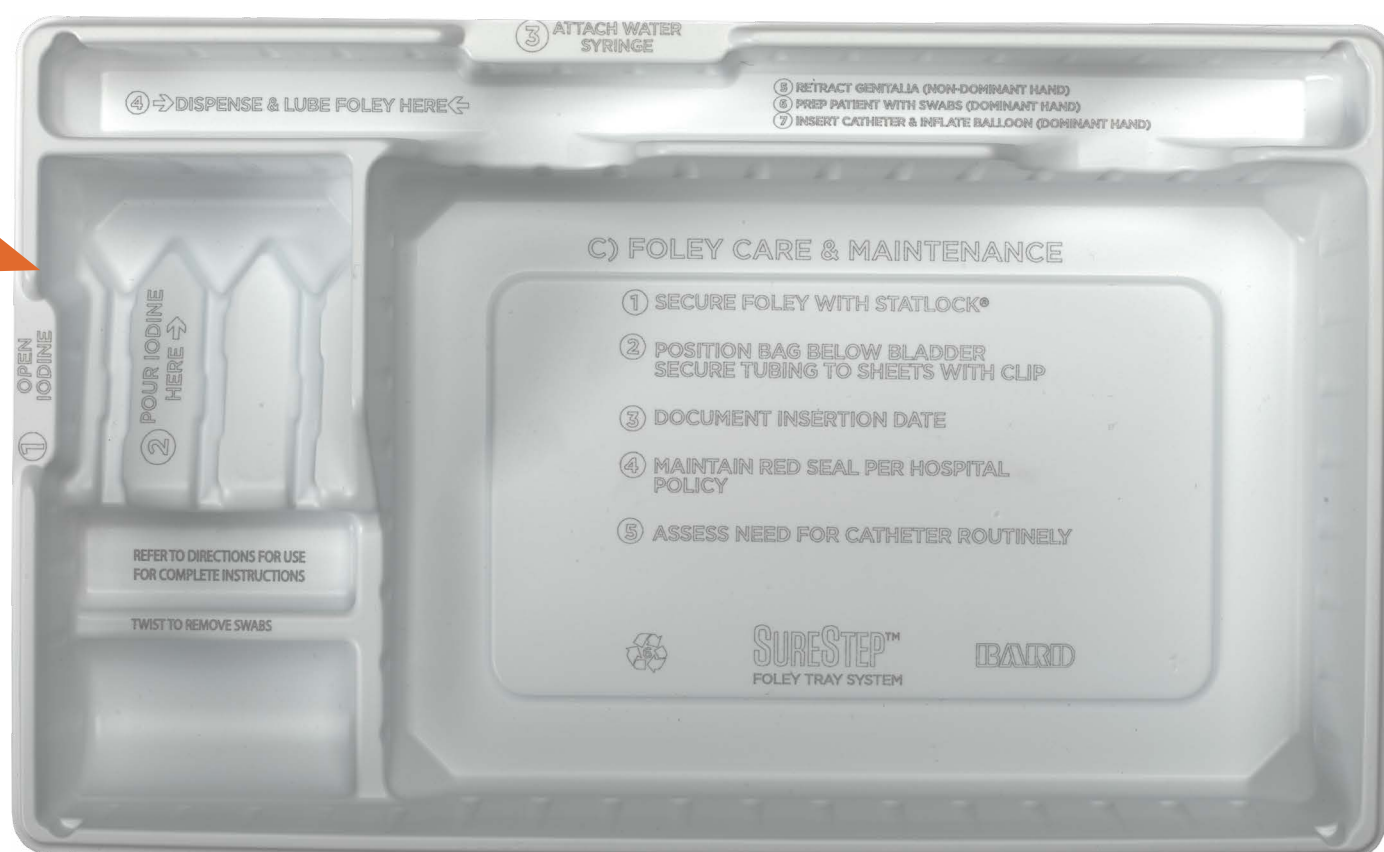

BARD | MEDICAL

C. R. Bard, Inc.
8195 Industrial Boulevard
Covington, GA 30014
1-800-526-4455
www.bardmedical.com

Foley catheters are intended for use in the drainage and/or collection and/or measurement of urine. STATLOCK[®] devices should be monitored daily and replaced when clinically indicated, at least every 7 days. Catheter insertion site should be treated per established hospital policy and procedure. STATLOCK[®] devices are contraindicated on patients with known tape or adhesive allergies.

Please consult product label and insert for any indications, contraindications, hazards, warnings, cautions and directions for use.